

ANSI S3.6-2004
(Revision of ANSI S3.6-1996)

AMERICAN NATIONAL STANDARD

Specification for Audiometers


ANSI S3.6-2004

Accredited Standards Committee S3, Bioacoustics

Standards Secretariat
Acoustical Society of America
35 Pinelawn Road, Suite 114 E
Melville, NY 11747-3177

The American National Standards Institute, Inc. (ANSI) is the national coordinator of voluntary standards development and the clearinghouse in the U.S.A. for information on national and international standards.

The Acoustical Society of America (ASA) is an organization of scientists and engineers formed in 1929 to increase and diffuse the knowledge of acoustics and to promote its practical applications.

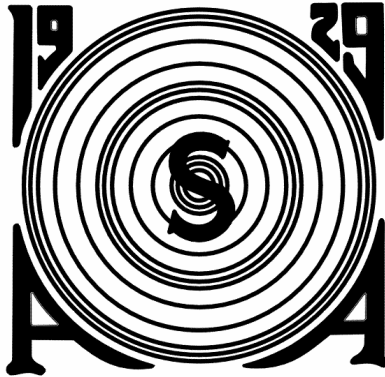

ANSI S3.6- 2004
(Revision of ANSI S3.6-1996)

AMERICAN NATIONAL STANDARD
Specification for Audiometers

Secretariat

Acoustical Society of America

Approval date: May 13, 2004

American National Standards Institute, Inc.

Abstract

The audiometers covered in this specification are devices designed for use in determining the hearing threshold level of an individual in comparison with a chosen standard reference threshold level. This standard provides specifications and tolerances for pure tone, speech, and masking signals and describes the minimum test capabilities of different types of audiometers.

AMERICAN NATIONAL STANDARDS ON ACOUSTICS

The Acoustical Society of America (ASA) provides the Secretariat for Accredited Standards Committees S1 on Acoustics, S2 on Mechanical Vibration and Shock, S3 on Bioacoustics, and S12 on Noise. These committees have wide representation from the technical community (manufacturers, consumers, trade associations, organizations with a general interest, and government representatives). The standards are published by the Acoustical Society of America as American National Standards after approval by their respective Standards Committees and the American National Standards Institute.


These standards are developed and published as a public service to provide standards useful to the public, industry, and consumers, and to Federal, State, and local governments.

Each of the accredited Standards Committees [operating in accordance with procedures approved by American National Standards Institute (ANSI)] is responsible for developing, voting upon, and maintaining or revising its own Standards. The ASA Standards Secretariat administers Committee organization and activity and provides liaison between the Accredited Standards Committees and ANSI. After the Standards have been produced and adopted by the Accredited Standards Committees, and approved as American National Standards by ANSI, the ASA Standards Secretariat arranges for their publication and distribution.

An American National Standard implies a consensus of those substantially concerned with its scope and provisions. Consensus is established when, in the judgment of the ANSI Board of Standards Review, substantial agreement has been reached by directly and materially affected interests. Substantial agreement means much more than a simple majority, but not necessarily unanimity. Consensus requires that all views and objections be considered and that a concerted effort be made towards their resolution.

The use of an American National Standard is completely voluntary. Their existence does not in any respect preclude anyone, whether he or she has approved the Standards or not, from manufacturing, marketing, purchasing, or using products, processes, or procedures not conforming to the Standards.

NOTICE: This American National Standard may be revised or withdrawn at any time. The procedures of the American National Standards Institute require that action be taken periodically to reaffirm, revise, or withdraw this Standard.



Acoustical Society of America
ASA Secretariat
35 Pinelawn Road, Suite 114E
Melville, New York 11747-3177
Telephone: 1 (631) 390-0215
Fax: 1 (631) 390-0217
E-mail: asastds@aip.org

© 2004 by Acoustical Society of America. This standard may not be reproduced in whole or in part in any form for sale, promotion, or any commercial purpose, or any purpose not falling within the provisions of the U.S. Copyright Act of 1976, without prior written permission of the publisher. For permission, address a request to the Standards Secretariat of the Acoustical Society of America.

Contents

1	Scope	1
1.1	Scope.....	1
1.2	Purpose.....	1
1.3	Applications	1
2	Normative references	1
3	Terms and definitions	3
4	Requirements for specific types of audiometers	7
4.1	Type designation.....	7
5	General requirements	8
5.1	Electrical Safety requirements.....	8
5.2	Acoustic Safety requirements.....	8
5.3	Power supply variation and environment conditions	8
5.3.1	Mains operation.....	8
5.3.2	Electrostatic or electromagnetic interference	10
5.3.3	Battery operation.....	10
5.3.4	Operating ranges for temperature and humidity	10
5.3.5	Test for conformity.....	10
5.4	Unwanted acoustic signals.....	11
5.4.1	General.....	11
5.4.2	Unwanted sounds from an earphone	11
5.4.3	Unwanted sound from a bone vibrator.....	12
5.4.4	Unwanted sound from an audiometer.....	12
5.5	Subject response system.....	12
5.6	Monitor earphone or loudspeaker.....	12
5.7	Talk back system	13
6	Signal sources	13
6.1	Pure-tone source.....	13
6.1.1	Frequencies and hearing levels	13
6.1.2	Rate of frequency change	13
6.1.3	Frequency modulated signals.....	13
6.1.4	Frequency accuracy	13
6.1.5	Harmonic distortion.....	14
6.2	Speech source.....	15
6.2.1	Clinical significance of speech audiometry	15
6.2.2	Free-field equivalent earphone output level	16

6.2.3	Uncorrected earphone output level	16
6.2.4	Loudspeaker output level	16
6.2.5	Free-field equivalent bone vibrator output level.....	16
6.2.6	Frequency response.....	16
6.2.7	Frequency response for recorded speech	16
6.2.8	Frequency response for microphone input	17
6.2.9	Overall distortion	17
6.2.10	Monitoring meter	17
6.2.11	Sound pressure level of speech signals	17
6.2.12	Standard reference sound pressure level for speech	18
6.3	Masking sounds.....	18
6.3.1	Narrow-band noise.....	18
6.3.2	White noise.....	18
6.3.3	Weighted random noise for the masking of speech.....	18
7	Signal level controls.....	19
7.1	Marking	19
7.2	Accuracy of sound pressure and vibratory force level	20
7.3	Hearing level control	20
7.3.1	Increments.....	20
7.3.2	Bekesy or automatic recording audiometers	20
7.3.3	Hearing level control linearity	20
7.4	Masking sound level control.....	21
7.4.1	Reference levels.	21
7.4.2	Accuracy of masking sound level.....	21
7.4.3	Maximal and range of adjustment of masking sound levels	21
7.5	Tone switching.....	21
7.5.1	Tone switch for manual audiometers	21
7.5.2	On/Off ratio for audiometers	22
7.5.3	Rise/fall times for audiometers	22
7.5.4	Pulsed tones for audiometers.....	22
7.5.5	Computer controlled, Bekesy, and automatic audiometers	22

8	Reference-signal facilities.....	22
8.1	Frequencies.....	23
8.2	Reference-signal level control.....	23
8.2.1	Range.....	23
8.2.2	Increments.....	23
8.2.3	Accuracy.....	23
8.2.4	Operation.....	24
9	Transducers (specifications, RETSPLs and RETFLs).....	24
9.1	Air conduction, supra-aural earphones.....	24
9.1.1	Characteristics of supra-aural earphones.....	24
9.1.2	Calibration.....	25
9.2	Air conduction, circumaural earphones.....	25
9.2.1	Headband.....	26
9.3	Air conduction, insert earphones.....	26
9.3.1	Reference levels in a occluded ear simulator.....	26
9.3.2	Reference levels in an HA -2 acoustic coupler with rigid tube attachment.....	27
9.3.3	Reference levels in an HA -1 acoustic coupler.....	28
9.4	Bone conduction.....	29
9.4.1	Bone vibrators.....	29
9.4.2	Headband.....	29
9.4.3	Reference equivalent threshold force levels (RETFLs).....	29
9.5	Sound field produced via loudspeakers.....	30
9.5.1	Sound field characteristics.....	30
10	Device marking and instruction manual.....	31
10.1	Marking.....	31
10.2	Instruction manual.....	31
Annex A	34
Annex B	36
Annex C	37
C.1	General.....	37
C.2	Calibration.....	37
C.3	Microphone.....	37
C.4	Adapters for making extended high frequency measurements on an IEC 60318-2 artificial ear.....	37
C.5	Coupler configurations using a Type 1 adapter.....	37
C.6	Coupler configuration using a Type 2 adapter.....	41
C.7	Environmental conditions.....	41
C.8	References.....	41
Annex D	42
D.1	General.....	42

D.2	Probe tube method.....	42
D.3	Loudness-balance method.....	43
D.4	Threshold-determination method.....	43
D.5	Standard reference earphone with other than specified coupler.....	43
D.6	Standard earphones with other than specified cushions.....	44
D.7	Earphone and coupler both different from standard types.....	44
Annex E	45
E.1	General.....	45
E.2	Reference levels.....	45
E.3	Vertical scale.....	45
E.4	Horizontal scale.....	45
E.5	Scale proportions.....	45
Annex F	46

Tables

NOTE The Table 2 given in previous editions of ANSI S3.6 has been eliminated in this edition. To avoid confusion, the other Tables in this edition were not renumbered.

Table 1	— Minimum required facilities for specific types of audiometers.....	9
Table 3	— Required frequencies and hearing levels for various audiometers.....	14
Table 4	— Maximum permissible harmonic distortion, expressed in percent.....	15
Table 5	— Narrow-band masking noise: upper and lower cut-off frequencies and correction factors for determining RETSPLs.....	19
Table 6	— Reference equivalent threshold sound pressure levels (RETSPLs) (dB re 20 μ Pa) for supra-aural earphones.....	25
Table 7	— Reference equivalent threshold sound pressure levels (RETSPLs) (dB re 20 μ Pa) for insert earphones.....	28
Table 8	— Reference equivalent threshold force levels (RETFs) for bone vibrators.....	30
Table 9	— Reference equivalent threshold sound pressure levels (RETSPLs) (dB re 20 μ Pa) for sound-field testing.....	32
Table A.1	— Difference between the free-field equivalent sensitivity level GF and the coupler or artificial ear level GC for two types of earphones.....	35
Table C.1	— Reference equivalent threshold sound pressure levels (RETSPLs)(dB re 20 μ Pa) for circumaural earphones.....	38

Figures

Figure 1	— Rise/fall envelope of test tones.....	23
Figure 2	— Coupling of the insert earphone to the calibration coupler. Figure 2(a) shows an occluded ear simulator (as described in ANSI 3.25 and IEC 60711) see subclause 9.3.1; Figure 2(b) an HA-2 acoustic coupler with rigid tube attachment (as described in ANSI 3.7, see subclause 9.3.2; and Figure 2(c) an HA-1 acoustic coupler (as described in ANSI S3.7), see subclause 9.3.3.....	27
Figure C.1	— 1 adaptor for use with IEC 60318-2 artificial ear.....	39
Figure C.2	— Position of Type 1 adapter on the IEC 60318-2 artificial ear.....	39
Figure C.3	— Type 2 adapter for use with IEC 60318-2 artificial ear.....	40
Figure C.4	— Position of Type 2 adapter on the IEC 60318-2 artificial ear.....	40
Figure F.1	— Earphone supra-aural cushion MX41/AR.....	46
Figure F.2	— Earphone supra-aural cushion Telephonic Type 51.....	47

Foreword

[*This Foreword is for information only, and is not a part of the American National Standard ANSI S3.6 - 2004 American National Standard Specification for Audiometers*].

This standard comprises a part of a group of definitions, standards, and specifications for use in bioacoustics. It was developed and approved by Accredited Standards Committee S3 Bioacoustics, under its approved operating procedures. Those procedures have been accredited by the American National Standards Institute (ANSI). The Scope of Accredited Standards Committee S3 is as follows:

Standards, specification, methods of measurements and test, and terminology in the fields of mechanical shock, and physical acoustics, including aspects of general acoustics, shock, and vibration that pertain to biological safety, tolerance, and comfort.

This standard is a revision of ANSI S3.6-1996, which has been technically revised to incorporate changes to keep this standard compatible with other equivalent international (IEC and ISO) standards. Table 2 has been deleted in this revision. The updated information formerly provided in this table can be found in IEC 60601-1.

This standard contains comparable information to current ISO Standards for pure tone thresholds, bone conduction and sound field.

At the time this Standard was submitted to Accredited Standards Committee S3, Bioacoustics for approval, the membership was as follows:

R.F. Burkard, *Chair*

C.A. Champlin, *Vice-Chair*
S.B. Blaeser, *Secretary*

Acoustical Society of America	R.F. Burkard
.....	C.A. Champlin (<i>Alt.</i>)
American Academy of Audiology	L. Shotland
.....	D.A. Fabry (<i>Alt.</i>)
American Academy of Otolaryngology, Head and Neck Surgery, Inc.	R.A. Dobie
.....	L.A. Michael (<i>Alt.</i>)
American Industrial Hygiene Association	J. Banach
.....	D. Driscoll (<i>Alt.</i>)
American Speech-Hearing-Language Association (ASHA)	G. Linn
.....	V. Gladstone (<i>Alt.</i>)
Audio Engineering Society, Inc.	R.H. Campbell
.....	M.R. Chial (<i>Alt.</i>)
Caterpillar, Inc.	D. Roley
.....	K.G. Meitl (<i>Alt.</i>)
Council for Accreditation in Occupational Hearing Conservation (CAOHC)	R.D. Bruce
.....	E.H. Berger (<i>Alt.</i>)

Hearing Industries Association	T.A. Victorian
.....	C.M. Rogin (<i>Alt.</i>)
Howard Leight Industries	V. Larson
.....	E. Woo (<i>Alt.</i>)
International Hearing Society	K. LaFerle
John Deere	L. DeVries
National Institute of Standards and Technology	V. Nedzelnitsky
.....	R. Wagner (<i>Alt.</i>)
Power Tool Institute	W.D. Spencer
.....	M. Hickok (<i>Alt.</i>)
U.S. Air Force	R. McKinley
.....	S.D. Smith (<i>Alt.</i>)
U.S. Army Aeromedical Research Lab	W. Ahroon
.....	N. Alem (<i>Alt.</i>)
U.S. Army CERL	L. Pater
.....	D. Delaney (<i>Alt.</i>)
U.S. Army Human Research & Engineering Directorate	T.R. Letowski
.....	P. Henry (<i>Alt.</i>)
U.S. Department of Transportation	E.D. Sussman
.....	T. Raslear (<i>Alt.</i>)
U.S. Department of the Air Force	R. McKinley
.....	S.D. Smith (<i>Alt.</i>)

Individual Experts of the Accredited Standards Committee S3, Bioacoustics, were:

J.R. Bareham	K.D. Kryter	P.D. Schomer
R.W. Benson	R. McKinley	H.E. von Gierke
A.J. Brammer	C.W. Nixon	D.E. Wasserman
A.J. Campanella	D.D. Reynolds	L.A. Wilber
J.L. Fletcher	J.D. Royster	W.A. Yost
T. Frank	L.H. Royster	

Working Group S3/WG35, Audiometers, which assisted Accredited Standards Committee S3, Bioacoustics, in the development of this standard, had the following membership.

R.L. Grason, Chair

S. Benson

T. Frank

R. Veillette

J. Forman

R. Grason

L.A. Wilber

S. Fournier

T.R. Letowski

Suggestions for improvements of this standard will be welcomed. They should be sent to Accredited Standards Committee S3, Bioacoustics, in care of the Standards Secretariat of the Acoustical Society of America, 35 Pinelawn Road, Suite 114E, Melville, New York 11747-3177. Telephone: 631-390-0215; FAX: 631-390-0217; E-mail: asastds@aip.org

This is a preview of "ANSI S3.6-2004". [Click here to purchase the full version from the ANSI store.](#)

American National Standard

Specification for Audiometers

1 Scope

1.1 Scope

Audiometers are electronic instruments intended for the testing of human hearing. This standard includes specifications and tolerances for audiometers and standard reference threshold levels for audiometric transducers such as supra-aural, circumaural, and insert earphones, bone vibrators, and loudspeakers.

This standard classifies audiometers according to the type of signal generated (pure tones, speech, or both), mode of operation, and complexity or range of auditory functions tested. Audiometers are also classified by type. Audiometers used for diagnostic assessment are classified as Types 1, 2, or 3 while audiometers having air-conduction facilities only are classified as Type 4.

1.2 Purpose

The purpose of this standard is to ensure that tests of hearing, and particularly tests of hearing threshold, performed on the same individual with different audiometers complying with this standard, shall give equivalent results when used under comparable test conditions. Further, the test results shall accurately and validly represent the level difference, if any, that may exist between the threshold of the individual tested and the reference threshold of hearing. This standard covers the general specifications for audiometers that require behavioral responses from a listener, as well as specific requirements governing the functional units of audiometric equipment such as type or types of signal, signal level control mechanisms, and types of transducers. In addition, instruments used primarily for non-audiometric purposes, but which may incorporate calibrated sound sources (e.g. acoustic immittance systems, otoacoustic emission recording devices, or narrow-band noise generators), shall, whenever possible, conform to clauses 4 through 10 of this standard.

1.3 Applications

This standard specifies requirements for audiometers used primarily to determine hearing threshold levels with respect to standard reference threshold levels.

2 Normative references

The following referenced documents are indispensable for the application of this standard. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ANSI S1.1-1994 (R 2004), *American National Standard Acoustical Terminology*.

ANSI S1.4-1983 (R 2001), *American National Standard Specification for Sound Level Meters*.

ANSI S3.1-1999 (R 2003), *American National Standard Maximum Permissible Ambient Noise Levels for Audiometric Test Rooms*.