


2015-07-06

Sterilisation af sundhedsprodukter – Bestråling – Del 1: Krav til udvikling, validering og rutinekontrol af en sterilisationsproces for medicinsk udstyr

Sterilization of health care products – Radiation –
Part 1: Requirements for development, validation and
routine control of a sterilization process for medical
devices (ISO 11137-1:2006, including Amd 1:2013)

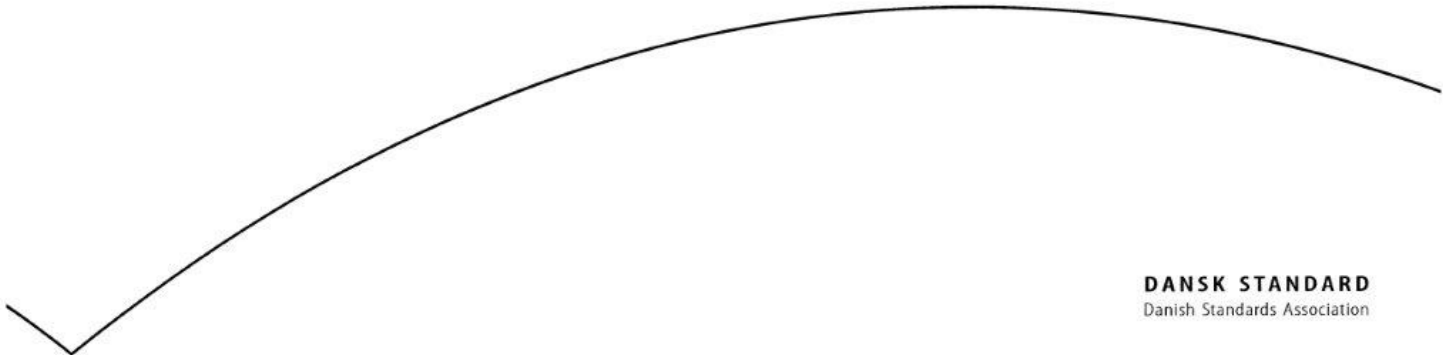

DANSK STANDARD
Danish Standards Association

Göteborg Plads 1
DK-2150 Nordhavn

Tel: +45 39 96 61 01

Fax: +45 39 96 61 02

dansk.standard@ds.dk

www.ds.dk

This is a preview of "DS/EN ISO 11137-1:20...". Click here to purchase the full version from the ANSI store.

DS-projekt: M250020
ICS: 11.080.01

Første del af denne publikations betegnelse er:

DS/EN ISO, hvilket betyder, at det er en international standard, der har status både som europæisk og dansk standard.

Denne publikations overensstemmelse er:

IDT med: ISO 11137-1:2006 + ISO 11137-1/Amd1:2013.

IDT med: EN ISO 11137-1:2015.

DS-publikationen er på engelsk.

Denne publikation erstatter: DS/EN ISO 11137-1:2006 og DS/EN ISO 11137-1/A1:2013.

2017-10-16: Den danske titel er d.d. rettet af redaktionelle årsager.

DS-publikationstyper

Dansk Standard udgiver forskellige publikationstyper.

Typen på denne publikation fremgår af forsiden.

Der kan være tale om:

Dansk standard

- standard, der er udarbejdet på nationalt niveau, eller som er baseret på et andet lands nationale standard, eller
- standard, der er udarbejdet på internationalt og/eller europæisk niveau, og som har fået status som dansk standard

DS-information

- publikation, der er udarbejdet på nationalt niveau, og som ikke har opnået status som standard, eller
- publikation, der er udarbejdet på internationalt og/eller europæisk niveau, og som ikke har fået status som standard, fx en teknisk rapport, eller
- europæisk præstandard

DS-håndbog

- samling af standarder, eventuelt suppleret med informativt materiale

DS-hæfte

- publikation med informativt materiale

Til disse publikationstyper kan endvidere udgives

- tillæg og rettelsesblade

DS-publikationsform

Publikationstyperne udgives i forskellig form som henholdsvis

- fuldtekstpublikation (publikationen er trykt i sin helhed)
- godkendelsesblad (publikationen leveres i kopi med et trykt DS-omslag)
- elektronisk (publikationen leveres på et elektronisk medie)

DS-betegnelse

Alle DS-publikationers betegnelse begynder med DS efterfulgt af et eller flere præfikser og et nr., fx **DS 383**, **DS/EN 5414** osv. Hvis der efter nr. er angivet et **A** eller **Cor**, betyder det, enten at det er et **tillæg** eller et **rettelsesblad** til hovedstandard, eller at det er indført i hovedstandard.

DS-betegnelse angives på forsiden.

Overensstemmelse med anden publikation:

Overensstemmelse kan enten være IDT, EQV, NEQ eller MOD

- **IDT:** Når publikationen er identisk med en given publikation.
- **EQV:** Når publikationen teknisk er i overensstemmelse med en given publikation, men præsentationen er ændret.
- **NEQ:** Når publikationen teknisk eller præsentationsmæssigt ikke er i overensstemmelse med en given standard, men udarbejdet på baggrund af denne.
- **MOD:** Når publikationen er modificeret i forhold til en given publikation.

This is a preview of "DS/EN ISO 11137-1:20...". [Click here to purchase the full version from the ANSI store.](#)

EUROPÄISCHE NORM

June 2015

ICS 11.080.01

Supersedes EN ISO 11137-1:2006

English Version

**Sterilization of health care products - Radiation - Part 1:
Requirements for development, validation and routine control of
a sterilization process for medical devices (ISO 11137-1:2006,
including Amd 1:2013)**

Stérilisation des produits de santé - Irradiation - Partie 1:
Exigences relatives à la mise au point, à la validation et au
contrôle de routine d'un procédé de stérilisation pour les
dispositifs médicaux (ISO 11137-1:2006, y compris Amd
1:2013)

Sterilisation von Produkten für die Gesundheitsfürsorge -
Strahlen - Teil 1: Anforderungen an die Entwicklung,
Validierung und Lenkung der Anwendung eines
Sterilisationsverfahrens für Medizinprodukte (ISO 11137-
1:2006, einschließlich Amd 1:2013)

This European Standard was approved by CEN on 20 May 2015.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

CEN-CENELEC Management Centre: Avenue Marnix 17, B-1000 Brussels

This is a preview of "DS/EN ISO 11137-1:20...". Click here to purchase the full version from the ANSI store.

Contents

Page

Foreword.....	3
Annex ZA (informative) Relationship between this European Standard and the Essential Requirements of EU Directive 90/385/EEC on active implantable medical devices	5
Annex ZB (informative) Relationship between this European Standard and the Essential Requirements of EU Directive 93/42/EEC on medical devices	6
Annex ZC (informative) Relationship between this European Standard and the Essential Requirements of EU Directive 98/79/EC on <i>in vitro</i> diagnostic medical devices.....	7

This is a preview of "DS/EN ISO 11137-1:20...". [Click here to purchase the full version from the ANSI store.](#)

Foreword

The text of ISO 11137-1:2006, including Amd 1:2013 has been prepared by Technical Committee ISO/TC 198 "Sterilization of health care products" of the International Organization for Standardization (ISO) and has been taken over as EN ISO 11137-1:2015 by Technical Committee CEN/TC 204 "Sterilization of medical devices" the secretariat of which is held by BSI.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by December 2015, and conflicting national standards shall be withdrawn at the latest by December 2015.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

This document supersedes EN ISO 11137-1:2006.

This document has been prepared under a mandate given to CEN by the European Commission and the European Free Trade Association, and supports essential requirements of EU Directives.

For relationship with EU Directives, see informative Annexes ZA, ZB, ZC, which are an integral part of this document.

The following referenced documents are indispensable for the application of this document. For undated references, the edition of the referenced document (including any amendments) listed below applies. For dated references, only the edition cited applies. However, for any use of this standard within the meaning of Annex ZA, ZB or ZC, the user should always check that any referenced document has not been superseded and that its relevant contents can still be considered the generally acknowledged state-of-art.

When an IEC or ISO standard is referred to in the ISO standard text, this should be understood as a normative reference to the corresponding EN standard, if available, and otherwise to the dated version of the ISO or IEC standard as listed below.

NOTE The way in which these referenced documents are cited in normative requirements determines the extent (in whole or in part) to which they apply.

Table — Correlation between normative references and dated EN and ISO standards

Normative references as listed in Clause 2 of the ISO standard	Equivalent dated standard	
	EN	ISO
ISO 10012-1	EN ISO 10012:2003	ISO 10012:2003
ISO 11137-2	EN ISO 11137-2:2013	ISO 11137-2:2013
ISO 11737-1	EN ISO 11737-1:2006 + AC:2009	ISO 11737-1:2006 + Cor 1:2007
ISO 11737-2	EN ISO 11737-2:2009	ISO 11737-2:2009
ISO 13485	EN ISO 13485:2012	ISO 13485:2003

This is a preview of "DS/EN ISO 11137-1:20...". [Click here to purchase the full version from the ANSI store.](#)

According to the CEN-CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

Endorsement notice

The text of ISO 11137-1:2006, including Amd 1:2013 has been approved by CEN as EN ISO 11137-1:2015 without any modification.

This is a preview of "DS/EN ISO 11137-1:20...". Click here to purchase the full version from the ANSI store.

Annex ZA (informative)

Relationship between this European Standard and the Essential Requirements of EU Directive 90/385/EEC on active implantable medical devices

This European Standard has been prepared under a mandate given to CEN/CENELEC by the European Commission and the European Free Trade Association to provide a means of conforming to Essential Requirements of the New Approach Directive 90/385/EEC on active implantable medical devices.

Once this standard is cited in the Official Journal of the European Union under that Directive and has been implemented as a national standard in at least one Member State, compliance with the normative clauses of this standard given in Table ZA.1 confers, within the limits of the scope of this standard, a presumption of conformity with the corresponding Essential Requirements of that Directive and associated EFTA regulations.

NOTE 1 Where a reference from a clause of this standard to the risk management process is made, the risk management process needs to be in compliance with 90/385/EEC, as amended by 2007/47/EC. This means that risks have to be reduced 'as far as possible', 'to a minimum', 'to the lowest possible level', 'minimized' or 'removed', according to the wording of the corresponding essential requirement.

NOTE 2 The manufacturer's policy for determining **acceptable risk** must be in compliance with essential requirements 1, 4, 5, 8, 9 and 10 of the Directive.

NOTE 3 This Annex ZA is based on normative references according to the table of references in the European foreword, replacing the references in the core text.

NOTE 4 When an Essential Requirement does not appear in Table ZA.1, it means that it is not addressed by this European Standard.

Table ZA.1 — Correspondence between this European Standard and Directive 90/385/EEC

Clauses of this EN	Essential Requirements (ERs) of Directive 90/385/EEC	Qualifying remarks/Notes
4,5,6,7,8,9,10,11,12	7	<p>Only a sterilization process using ionizing radiation is considered by this standard.</p> <p>This relevant Essential Requirement is only partly addressed in this European Standard. Design and packaging for maintenance of sterility during transportation and storage are not covered. Aspects of manufacture other than those related to sterilization are not covered.</p>

WARNING — Other requirements and other EU Directives may be applicable to the product(s) falling within the scope of this Standard.

This is a preview of "DS/EN ISO 11137-1:20...". Click here to purchase the full version from the ANSI store.

Annex ZB
(informative)

Relationship between this European Standard and the Essential Requirements of EU Directive 93/42/EEC on medical devices

This European Standard has been prepared under a mandate given to CEN/CENELC by the European Commission and the European Free Trade Association to provide a means of conforming to Essential Requirements of the New Approach Directive 93/42/EEC on medical devices.

Once this standard is cited in the Official Journal of the European Union under that Directive and has been implemented as a national standard in at least one Member State, compliance with the normative clauses of this standard given in Table ZB.1 confers, within the limits of the scope of this standard, a presumption of conformity with the corresponding Essential Requirements of that Directive and associated EFTA regulations.

NOTE 1 Where a reference from a clause of this standard to the risk management process is made, the risk management process needs to be in compliance with 93/42/EEC, as amended by 2007/47/EC. This means that risks have to be reduced 'as far as possible', 'to a minimum', 'to the lowest possible level', 'minimized' or 'removed', according to the wording of the corresponding essential requirement.

NOTE 2 The manufacturer's policy for determining **acceptable risk** must be in compliance with essential requirements 1, 2, 5, 6, 7, 8, 9, 11 and 12 of the Directive.

NOTE 3 This Annex ZA is based on normative references according to the table of references in the European foreword, replacing the references in the core text.

NOTE 4 When an Essential Requirement does not appear in Table ZA.1, it means that it is not addressed by this European Standard.

Table ZB.1 — Correspondence between this European Standard and Directive 93/42/EEC

Clauses of this EN	Essential Requirements (ERs) of Directive 93/42/EEC	Qualifying remarks/Notes
4,5,6,7,8,9,10,11,12	8.3	Only a sterilization process using ionizing radiation is considered by this standard. This relevant Essential Requirement is only partly addressed in this European Standard. Design and packaging for maintenance of sterility during transportation and storage are not covered. Aspects of manufacture other than those related to sterilization are not covered.
4,5,6,7,8,9,10,11,12	8.4	This relevant Essential Requirement is only partly addressed in this European Standard. Aspects of manufacture other than those related to sterilization are not covered.

WARNING — Other requirements and other EU Directives may be applicable to the product(s) falling within the scope of this Standard.

This is a preview of "DS/EN ISO 11137-1:20...". Click here to purchase the full version from the ANSI store.

Annex ZC (informative)

Relationship between this European Standard and the Essential Requirements of EU Directive 98/79/EC on *in vitro* diagnostic medical devices

This European Standard has been prepared under a mandate given to CEN/CENELEC by the European Commission and the European Free Trade Association to provide a means of conforming to Essential Requirements of the New Approach Directive 98/79/EC on *in vitro* diagnostic medical devices.

Once this standard is cited in the Official Journal of the European Union under that Directive and has been implemented as a national standard in at least one Member State, compliance with the normative clauses of this standard given in Table ZC.1 confers, within the limits of the scope of this standard, a presumption of conformity with the corresponding Essential Requirements of that Directive and associated EFTA regulations.

NOTE 1 Where a reference from a clause of this standard to the risk management process is made, the risk management process needs to be in compliance with 98/79/EC. This means that risks have to be reduced 'as far as possible', 'to a minimum', 'to the lowest possible level', 'minimized' or 'removed', according to the wording of the corresponding essential requirement.

NOTE 2 The manufacturer's policy for determining **acceptable risk** must be in compliance with essential requirements Part A: 1, 2 and 5; Part B: 1.2, 2, 3, 5, 6, and 7 of the Directive.

NOTE 3 This Annex ZA is based on normative references according to the table of references in the European foreword, replacing the references in the core text.

NOTE 4 When an Essential Requirement does not appear in Table ZA.1, it means that it is not addressed by this European Standard.

Table ZC.1 — Correspondence between this European Standard and Directive 98/79/EC

Clauses of this EN	Essential Requirements (ERs) of Directive 98/79/EC	Qualifying remarks/Notes
4,5,6,7,8,9,10,11,12	B.2.3	<p>Only a sterilization process using ionizing radiation is considered by this standard.</p> <p>This relevant Essential Requirement is only partly addressed in this European Standard. Design and packaging for maintenance of sterility during transportation and storage are not covered. Aspects of manufacture other than those related to sterilization are not covered.</p>

This is a preview of "DS/EN ISO 11137-1:20...". [Click here to purchase the full version from the ANSI store.](#)

4,5,6,7,8,9,10,11,12	B.2.4	This relevant Essential requirement is addressed only with regard to: - sterilization, not covering other special microbiological state - devices for which sterilization by radiation is appropriate
----------------------	-------	---

WARNING — Other requirements and other EU Directives may be applicable to the product(s) falling within the scope of this Standard.

First edition
2006-04-15

Sterilization of health care products — Radiation —

Part 1:

Requirements for development, validation and routine control of a sterilization process for medical devices

Stérilisation des produits de santé — Irradiation —

*Partie 1: Exigences relatives à la mise au point, à la validation et au
contrôle de routine d'un procédé de stérilisation pour les dispositifs
médicaux*



Reference number
ISO 11137-1:2006(E)

© ISO 2006

This is a preview of "DS/EN ISO 11137-1:20...". [Click here to purchase the full version from the ANSI store.](#)

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

© ISO 2006

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

This is a preview of "DS/EN ISO 11137-1:20...". Click here to purchase the full version from the ANSI store.

Contents

Page

Foreword.....	iv
Introduction	v
1 Scope	1
2 Normative references	2
3 Terms and definitions.....	2
4 Quality management system elements	8
4.1 Documentation	8
4.2 Management responsibility	9
4.3 Product realization.....	9
4.4 Measurement, analysis and improvement — Control of nonconforming product	9
5 Sterilizing agent characterization	9
5.1 Sterilizing agent	9
5.2 Microbicidal effectiveness	9
5.3 Material effects.....	9
5.4 Environmental considerations	10
6 Process and equipment characterization	10
6.1 Process	10
6.2 Equipment	10
7 Product definition	11
8 Process definition.....	12
8.1 Establishing the maximum acceptable dose	12
8.2 Establishing the sterilization dose.....	12
8.3 Specifying the maximum acceptable dose and the sterilization dose.....	13
8.4 Transference of maximum acceptable, verification or sterilization dose between radiation sources	13
9 Validation.....	14
9.1 Installation qualification.....	14
9.2 Operational qualification.....	14
9.3 Performance qualification.....	15
9.4 Review and approval of validation.....	15
10 Routine monitoring and control	16
11 Product release from sterilization.....	17
12 Maintaining process effectiveness	17
12.1 Demonstration of continued effectiveness	17
12.2 Recalibration	20
12.3 Maintenance of equipment	20
12.4 Requalification of equipment	20
12.5 Assessment of change.....	20
Annex A (informative) Guidance	21
Bibliography	36

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 11137-1 was prepared by Technical Committee ISO/TC 198, *Sterilization of health care product*.

This first edition, together with ISO 11137-2 and ISO 11137-3, cancels and replaces ISO 11137:1995.

ISO 11137 consists of the following parts, under the general title *Sterilization of health care products — Radiation*:

- *Part 1: Requirements for development, validation and routine control of a sterilization process for medical devices*
- *Part 2: Establishing the sterilization dose*
- *Part 3: Guidance on dosimetric aspects*

Introduction

A sterile medical device is one that is free of viable microorganisms. International Standards, which specify requirements for validation and routine control of sterilization processes, require, when it is necessary to supply a sterile medical device, that adventitious microbiological contamination of a medical device prior to sterilization be minimized. Even so, medical devices produced under standard manufacturing conditions in accordance with the requirements for quality management systems (see, for example, ISO 13485) may, prior to sterilization, have microorganisms on them, albeit in low numbers. Such medical devices are non-sterile. The purpose of sterilization is to inactivate the microbiological contaminants and thereby transform the non-sterile medical devices into sterile ones.

The kinetics of inactivation of a pure culture of microorganisms by physical and/or chemical agents used to sterilize medical devices can generally best be described by an exponential relationship between the numbers of microorganisms surviving and the extent of treatment with the sterilizing agent; inevitably this means that there is always a finite probability that a microorganism may survive regardless of the extent of treatment applied. For a given treatment, the probability of survival is determined by the number and resistance of microorganisms and by the environment in which the organisms exist during treatment. It follows that the sterility of any one medical device in a population subjected to sterilization processing cannot be guaranteed and the sterility of a processed population is defined in terms of the probability of there being a viable microorganism present on a medical device.

This part of ISO 11137 describes requirements that, if met, will provide a radiation sterilization process intended to sterilize medical devices, that has appropriate microbicidal activity. Furthermore, compliance with the requirements ensures that this activity is both reliable and reproducible so that predictions can be made, with reasonable confidence, that there is a low level of probability of there being a viable microorganism present on product after sterilization. Specification of this probability is a matter for regulatory authorities and may vary from country to country (see, for example, EN 556-1 and ANSI/AAMI ST67).

Generic requirements of the quality management system for design and development, production, installation and servicing are given in ISO 9001 and particular requirements for quality management systems for medical device production are given in ISO 13485. The standards for quality management systems recognise that, for certain processes used in manufacturing, the effectiveness of the process cannot be fully verified by subsequent inspection and testing of the product. Sterilization is an example of such a process. For this reason, sterilization processes are validated for use, the performance of the sterilization process is monitored routinely and the equipment is maintained.

Exposure to a properly validated, accurately controlled sterilization process is not the only factor associated with the provision of reliable assurance that the products are sterile and, in this regard, suitable for its intended use. Attention is therefore given to a number of considerations including:

- a) the microbiological status of incoming raw materials and/or components;
- b) the validation and routine control of any cleaning and disinfection procedures used on the product;
- c) the control of the environment in which the product is manufactured, assembled and packaged;
- d) the control of equipment and processes;
- e) the control of personnel and their hygiene;
- f) the manner and materials in which the product is packaged;
- g) the conditions under which product is stored.

This is a preview of "DS/EN ISO 11137-1:20...". [Click here to purchase the full version from the ANSI store.](#)

This part of ISO 11137 describes the requirements for ensuring that the activities associated with the process of radiation sterilization are performed properly. These activities are described in documented work programmes designed to demonstrate that the radiation process will consistently yield sterile products on treatment with doses falling within the predetermined limits.

The requirements are the normative parts of this part of ISO 11137 with which compliance is claimed. The guidance given in the informative annexes is not normative and is not provided as a checklist for auditors. The guidance provides explanations and methods that are regarded as being a suitable means for complying with the requirements. Methods other than those given in the guidance may be used, if they are effective in achieving compliance with the requirements of this part of ISO 11137.

The development, validation and routine control of a sterilization process comprise a number of discrete but interrelated activities; e.g. calibration, maintenance, product definition, process definition, installation qualification, operational qualification and performance qualification. While the activities required by this part of ISO 11137 have been grouped together and are presented in a particular order, this part of ISO 11137 does not require that the activities be performed in the order that they are presented. The activities required are not necessarily sequential, as the programme of development and validation may be iterative. It is possible that performing these different activities will involve a number of separate individuals and/or organizations, each of whom undertake one or more of these activities. This part of ISO 11137 does not specify the particular individuals or organizations to carry out the activities.

This is a preview of "DS/EN ISO 11137-1:20...". [Click here to purchase the full version from the ANSI store.](#)

Sterilization of health care products — Radiation —

Part 1:

Requirements for development, validation and routine control of a sterilization process for medical devices

1 Scope

1.1 This part of ISO 11137 specifies requirements for the development, validation and routine control of a radiation sterilization process for medical devices.

NOTE Although the scope of this part of ISO 11137 is limited to medical devices, it specifies requirements and provides guidance that may be applicable to other products and equipment.

This part of ISO 11137 covers radiation processes employing irradiators using,

- a) the radionuclide ^{60}Co or ^{137}Cs ,
 - b) a beam from an electron generator
- or
- c) a beam from an X-ray generator.

1.2 This part of ISO 11137 does not specify requirements for development, validation and routine control of a process for inactivating the causative agents of spongiform encephalopathies such as scrapie, bovine spongiform encephalopathy and Creutzfeld-Jakob disease. Specific recommendations have been produced in particular countries for the processing of materials potentially contaminated with these agents.

NOTE See, for example, ISO 22442-1, ISO 22442-2 and ISO 22442-3.

1.2.1 This part of ISO 11137 does not detail specified requirements for designating a medical device as sterile.

NOTE Attention is drawn to regional and national requirements for designating medical devices as “sterile.” See, for example, EN 556-1 or ANSI/AAMI ST67.

1.2.2 This part of ISO 11137 does not specify a quality management system for the control of all stages of production of medical devices.

NOTE It is not a requirement of this part of ISO 11137 to have a complete quality management system during manufacture, but the elements of a quality management system that are the minimum necessary to control the sterilization process are normatively referenced at appropriate places in the text (see, in particular, Clause 4). Attention is drawn to the standards for quality management systems (see ISO 13485) that control all stages of production of medical devices, including the sterilization process. Regional and national regulations for the provision of medical devices might require implementation of a complete quality management system and the assessment of that system by a third party.

1.2.3 This part of ISO 11137 does not require that biological indicators be used for validation or monitoring of radiation sterilization, nor does it require that a pharmacopoeial test for sterility be carried out for product release.

This is a preview of "DS/EN ISO 11137-1:20...". [Click here to purchase the full version from the ANSI store.](#)

1.2.4 This part of ISO 11137 does not specify requirements for occupational safety associated with the design and operation of irradiation facilities.

NOTE Attention is also drawn to the existence, in some countries, of regulations laying down safety requirements for occupational safety related to radiation.

1.2.5 This part of ISO 11137 does not specify requirements for the sterilization of used or reprocessed devices.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 10012-1, *Quality assurance requirements for measuring equipment — Part 1: Metrological confirmation system for measuring equipment*

ISO 11137-2:2006, *Sterilization of health care products — Radiation — Part 2: Establishing the sterilization dose*

ISO 11737-1, *Sterilization of medical devices — Microbiological methods — Part 1: Determination of a population of microorganisms on products*

ISO 11737-2, *Sterilization of medical devices — Microbiological methods — Part 2: Tests of sterility performed in the validation of a sterilization process*

ISO 13485:2003, *Medical devices — Quality management systems — Requirements for regulatory purposes*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1 absorbed dose dose

quantity of ionizing radiation energy imparted per unit mass of a specified material

NOTE 1 The unit of absorbed dose is the gray (Gy) where 1 Gy is equivalent to the absorption of 1 J/kg.

NOTE 2 For the purposes of this part of ISO 11137, the term dose is used to mean "absorbed dose".

3.2 bioburden

population of viable microorganisms on or in the product and/or sterile barrier system

[ISO/TS 11139:2006]

3.3 biological indicator

test system containing viable microorganisms providing a defined resistance to a specified sterilization process

[ISO/TS 11139:2006]